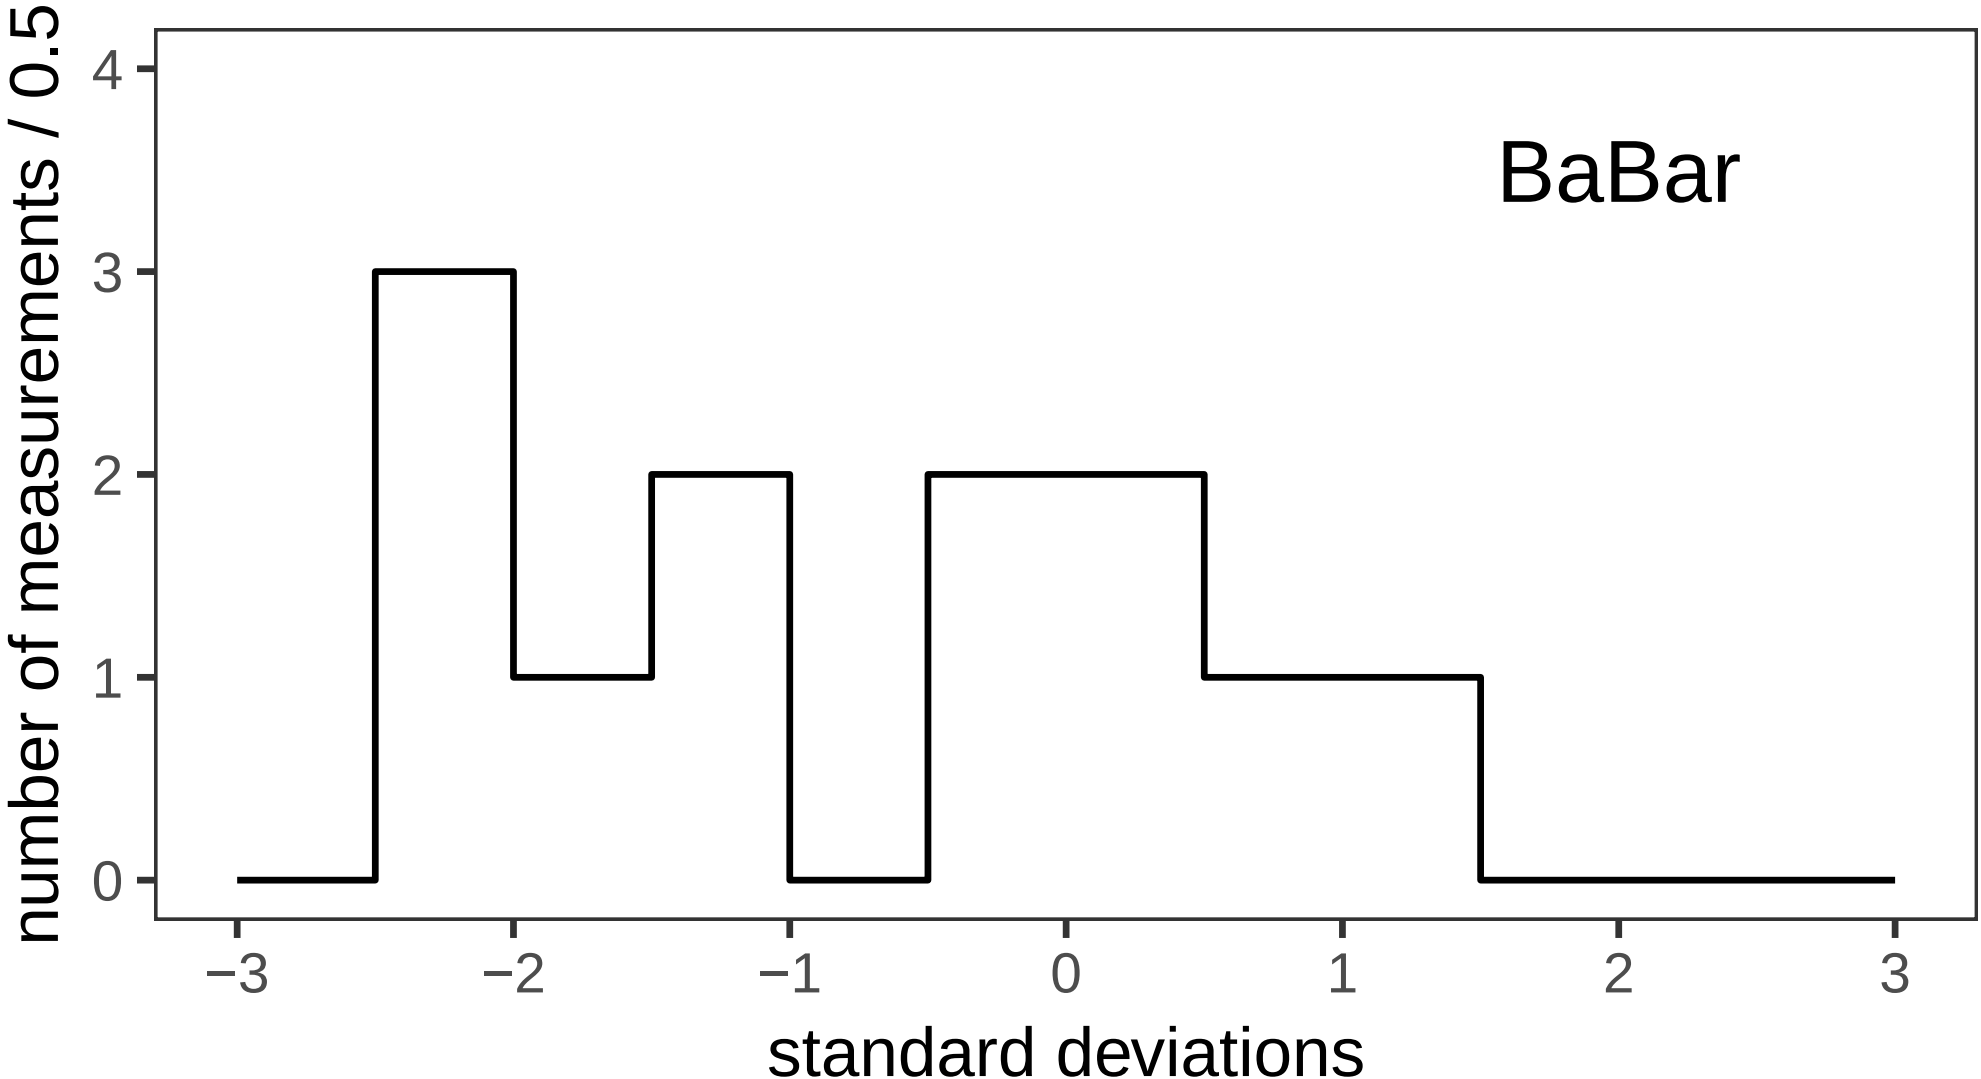
BaBar
number of measurements / 0.5
standard deviations
0
1
2
3
4
−3
−2
−1
0
1
2
3